

# Knobbe Martens Olson & Bear LLP

Intellectual Property Law



10/020002

2040 Main Street  
Fourteenth Floor  
Irvine, CA 92614  
Tel 949-760-0404  
Fax 949-760-9502  
www.kmob.com

Mark J. Kertz

September 29, 2005

Commissioner for Patents  
P.O. Box 1450  
Alexandria, VA 22313-1450

**Certificate**  
**OCT 07 2005**  
**of Correction**

Re: METHOD OF IMPLANTING AN INTRAOCULAR  
LENS SYSTEM  
Letters Patent No. 6,899,732  
Issued: May 31, 2005  
Our Reference: VGEN.010A

Dear Sir:

Enclosed for filing is a Certificate of Correction in connection with the above-identified patent.

As the error cited in the Certificate of Correction was incurred through no fault of the Patent Office, enclosed is our check in the amount of \$100. Please charge any additional fees to our Deposit Account No. 11-1410.

An explanation of the error and the corrections is set forth below.

Figures 18 and 19 are described at Column 15, line 60 to Column 16, line 45. Figures 18 and 19 are depicted below:

10/04/2005 AKELECH1 00000014 6899732

01 FC:1811

100.00 OP

OCT 12 2005

San Diego  
619-235-8550


San Francisco  
415-954-4114

Los Angeles  
310-551-3450


Riverside  
951-781-9231

San Luis Obispo  
805-547-5580

Commissioner of Patents,  
September 29, 2005  
Page -2-

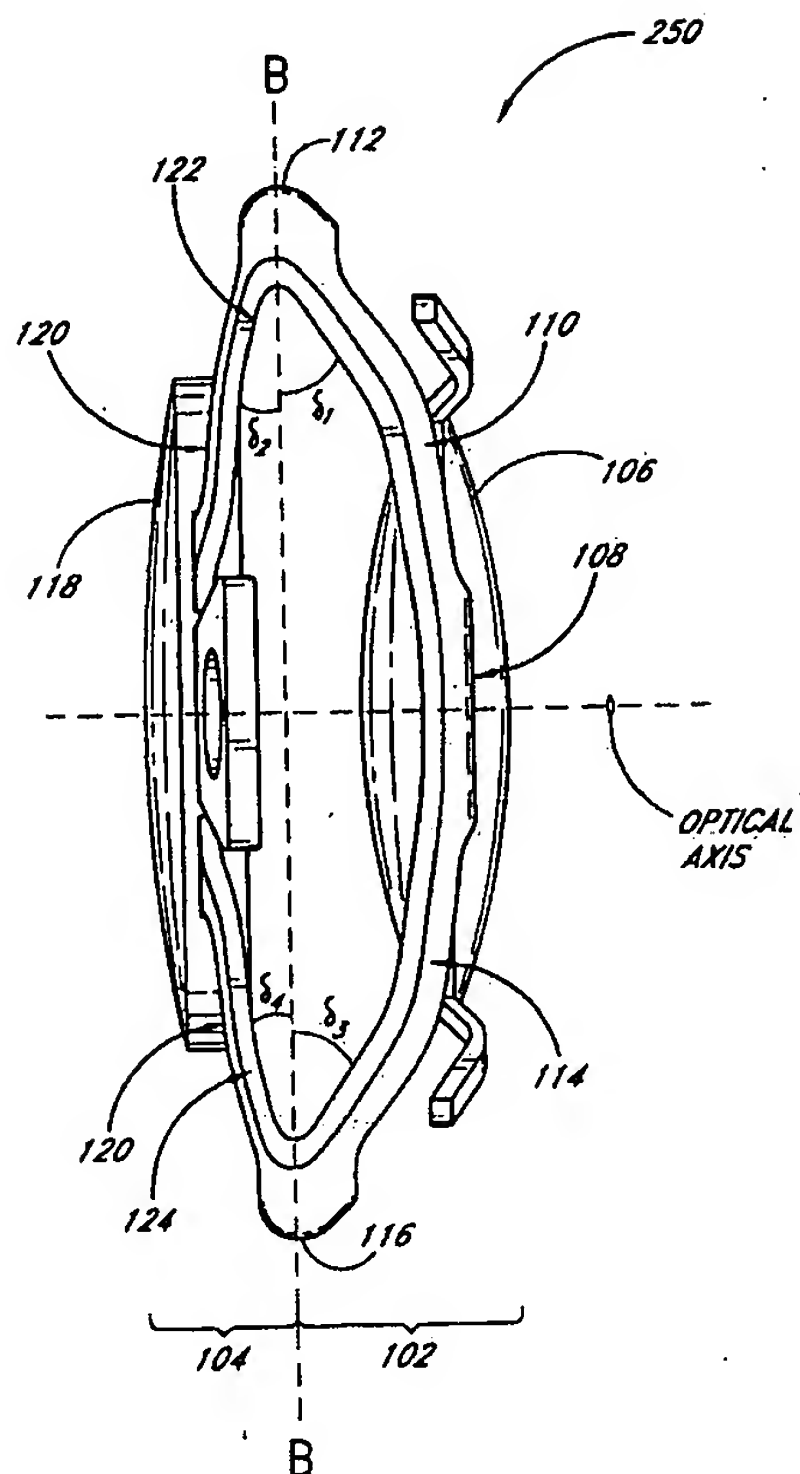

**FIG. 18**

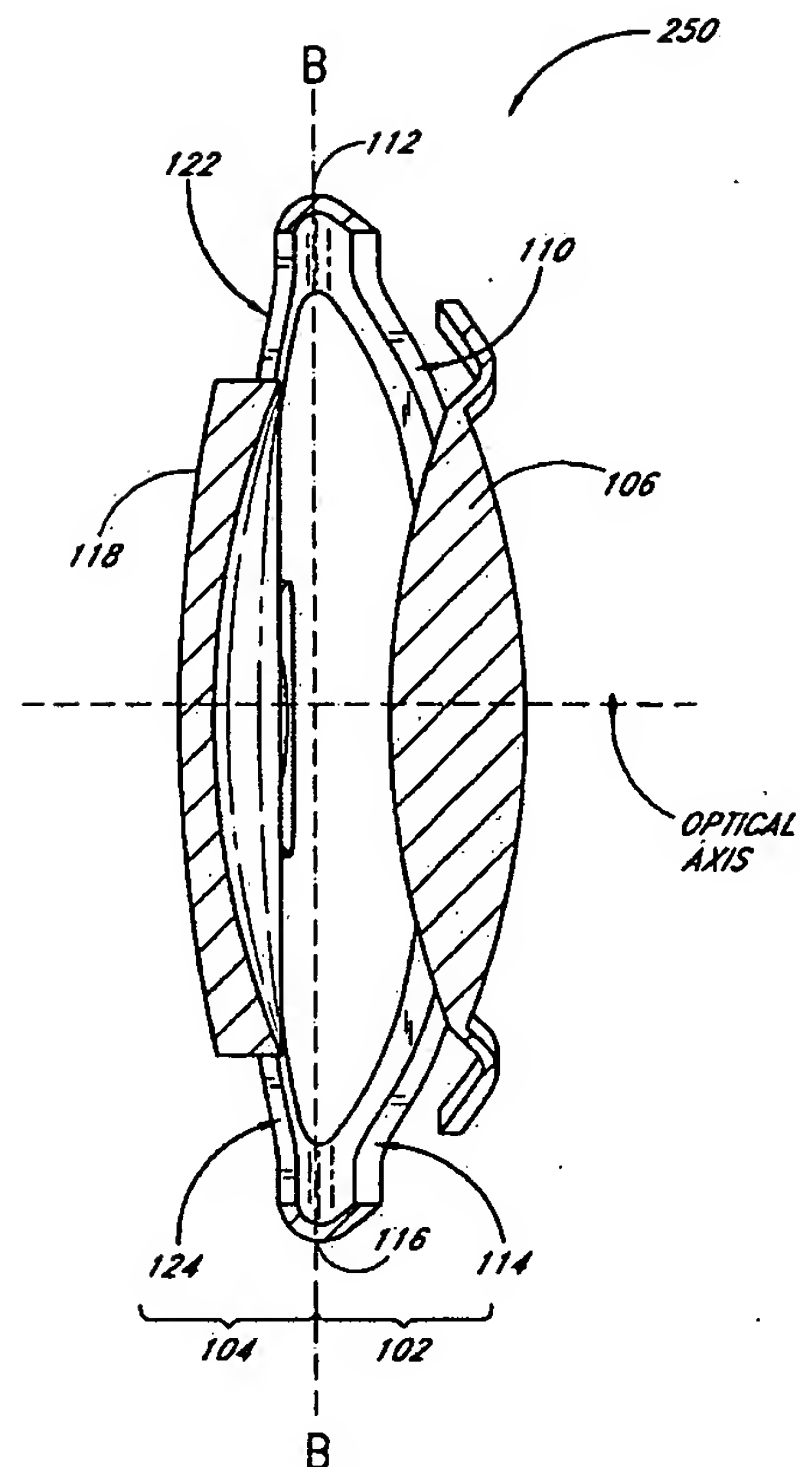

**FIG. 19**

The textual descriptions of Figures 18 and 19 contain a minor, obvious error at Column 16, line 12, in that the angles shown at the bottom of the lens system of Figures 18 and 19 are described as being substantially equal. Obviously, they are not. Indeed, the remainder of the description makes it abundantly clear that what is being described is a lens having asymmetry as viewed from the side, and that is exactly what the Figures depict. The correction to the specification made in the enclosed Certificate of Correction properly describes the angles as being unequal, and makes line 12 consistent with the other 53 lines of text that describe Figures 18 and 19, as well as with the figures themselves.

Respectfully submitted,

Knobbe, Martens, Olson & Bear, LLP

*Mark Kertz*

Mark J. Kertz  
Registration No. 43,711  
Customer No. 20,995

Enclosures

1912379:cb 090205

OCT 12 2005

# UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

**PATENT NO. :** 6,899,732

**DATED :** May 31, 2005

**INVENTOR(S):** Gholam Zadno-Azizi, et al.

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the specification, Col. 16, Line 12, delete “substantially equal” and substitute --unequal--.

MAILING ADDRESS OF SENDER:

Mark J. Kertz  
KNOBBE, MARTENS, OLSON & BEAR, LLP  
2040 Main Street, 14<sup>th</sup> Floor  
Irvine, California 92614

PATENT NO. 6,899,732